

SOP 45 | Advanced administration

Read device and tracking insights

Inspect aggregate quality patterns without overinterpreting small cohorts.

For Web · Administrator

Before you start Authorized insight access is required.

Open Manage > Device & research tools

Step 1 Open the insight screen

Select Device & tracking insights from authorized administration tools.

Step 2 Set the available filters

Choose property and the available device, platform or time filters. Read the cohort counts.

Step 3 Interpret the quality measures

Compare accuracy, freshness, permission, sync and device dimensions together. Respect suppressed or unknown results.

Step 4 Investigate a supported issue

Use an authorized run review or Operational support for a concrete failure. Preserve the distinction between device quality and employee performance.


Check your result You can describe the supported quality pattern and any limitations of the cohort.

If something goes wrong Small cohorts may be withheld. Missing or degraded evidence cannot be converted into an exact indoor visit claim.

See the picture reference on the next page.

SOP 45 Picture reference

Read device and tracking insights

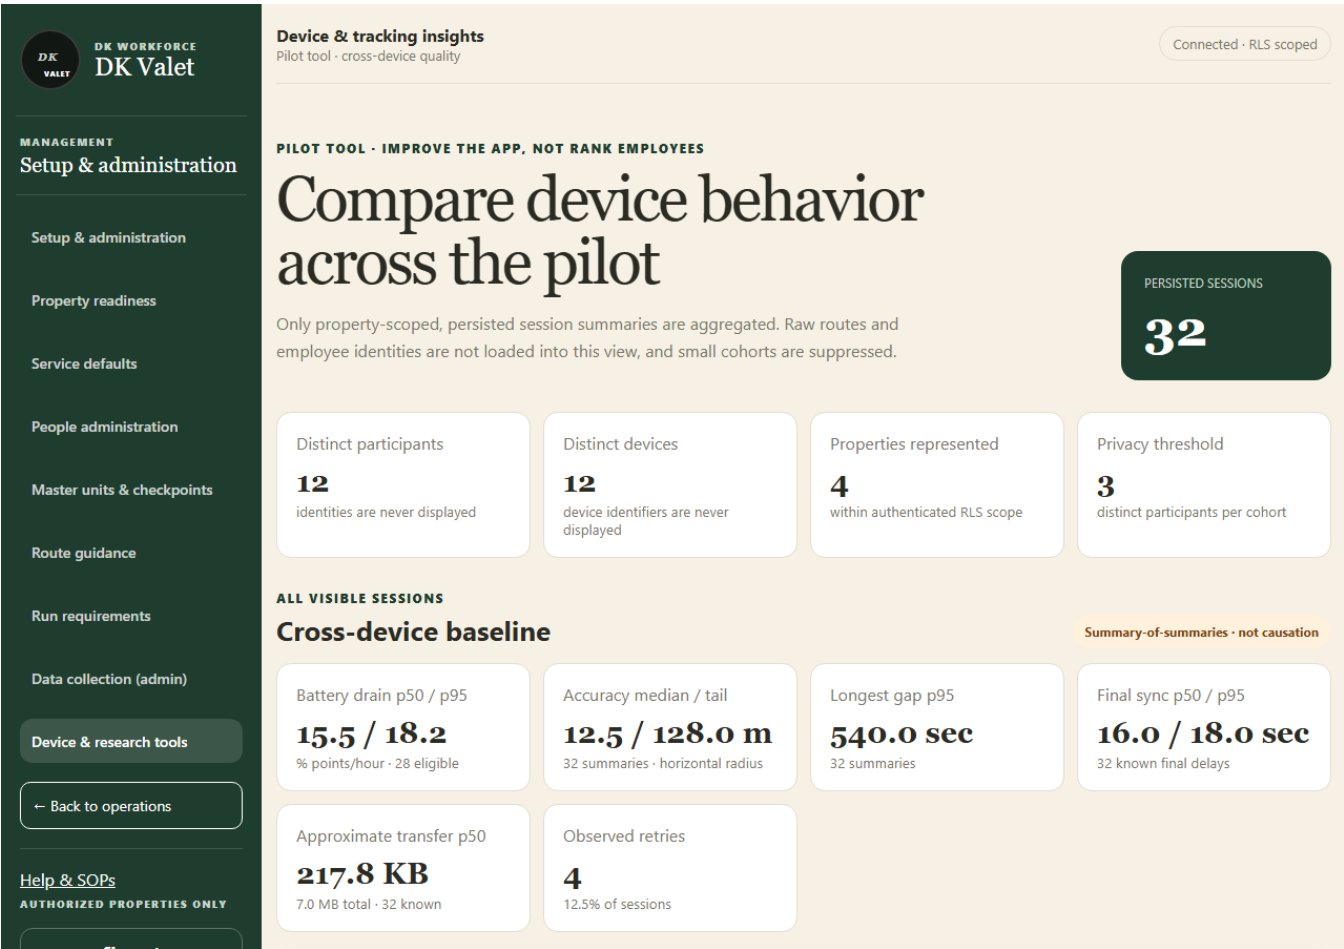

Step 2 · Compare device behavior across the pilot: use the property selector and the task controls shown.
Application screenshot with training data.